



Title:

Certificate of Analysis (CoA)

Date: 8/27/2026

Date Tested: 8/26/2026

Customer: Encore Aminos

Testing material: Selank

Lot Number: VECKCGAE

Sample ID: BTL261137-020

Content/Potency: 5 mg

Storage: R.T.

Visual Description: Small clear vial: white sample, white label, silver crimp, clear green plastic cap.

Labeled as: Selank

Manufacturer: Encore Aminos

Testing Purpose: FTIR and HPLC analysis for the identification, purity, potency and composition of a peptide product. It does not provide information on particulate matter, microbial contamination or presence of endotoxins.



Test	Method	Specification	Result
General Appearance	USP <630>	white powder	white powder
Mass	USP <41>	As recorded	28.9 mg
FTIR Identification and Composition Analysis	USP <197A>	Sample spectrum should confirm the content of peptide via characteristic bands	FTIR sample spectrum confirms the presence of Selank with addition of excipient(s)/fillers.
HPLC Purity of Peptide Assay	USP <621>	Specifications: $\geq 98\%$	99.7 %
HPLC Potency Assay	USP <621>	Specifications: 90 – 110% of 5 mg	5.7 mg (113.8 %)
Peptide-to-Excipients Ratio	USP <1151>	Recommended ratios of (1:0) to (1:10) for (peptide: excipients)	5.7 : 23.2 mg (1:4.1)

The results of the CoA relate only to the item(s) tested and applied to the sample as received.

Andrea Castro, BS
Scientist-II
BTLabsEscarlet Cabrieles, BS
Scientist-II
BTLabs

5601 Corporate Way | Suite 206 | West Palm Beach, FL 33407

Phone: (561) 625-0133


E-mail: info@btlabtesting.com | Website: <https://btlabtesting.com>




Title:

Certificate of Analysis (CoA)

FTIR ID and Composition Analysis: Selank Lot VECKCGAE

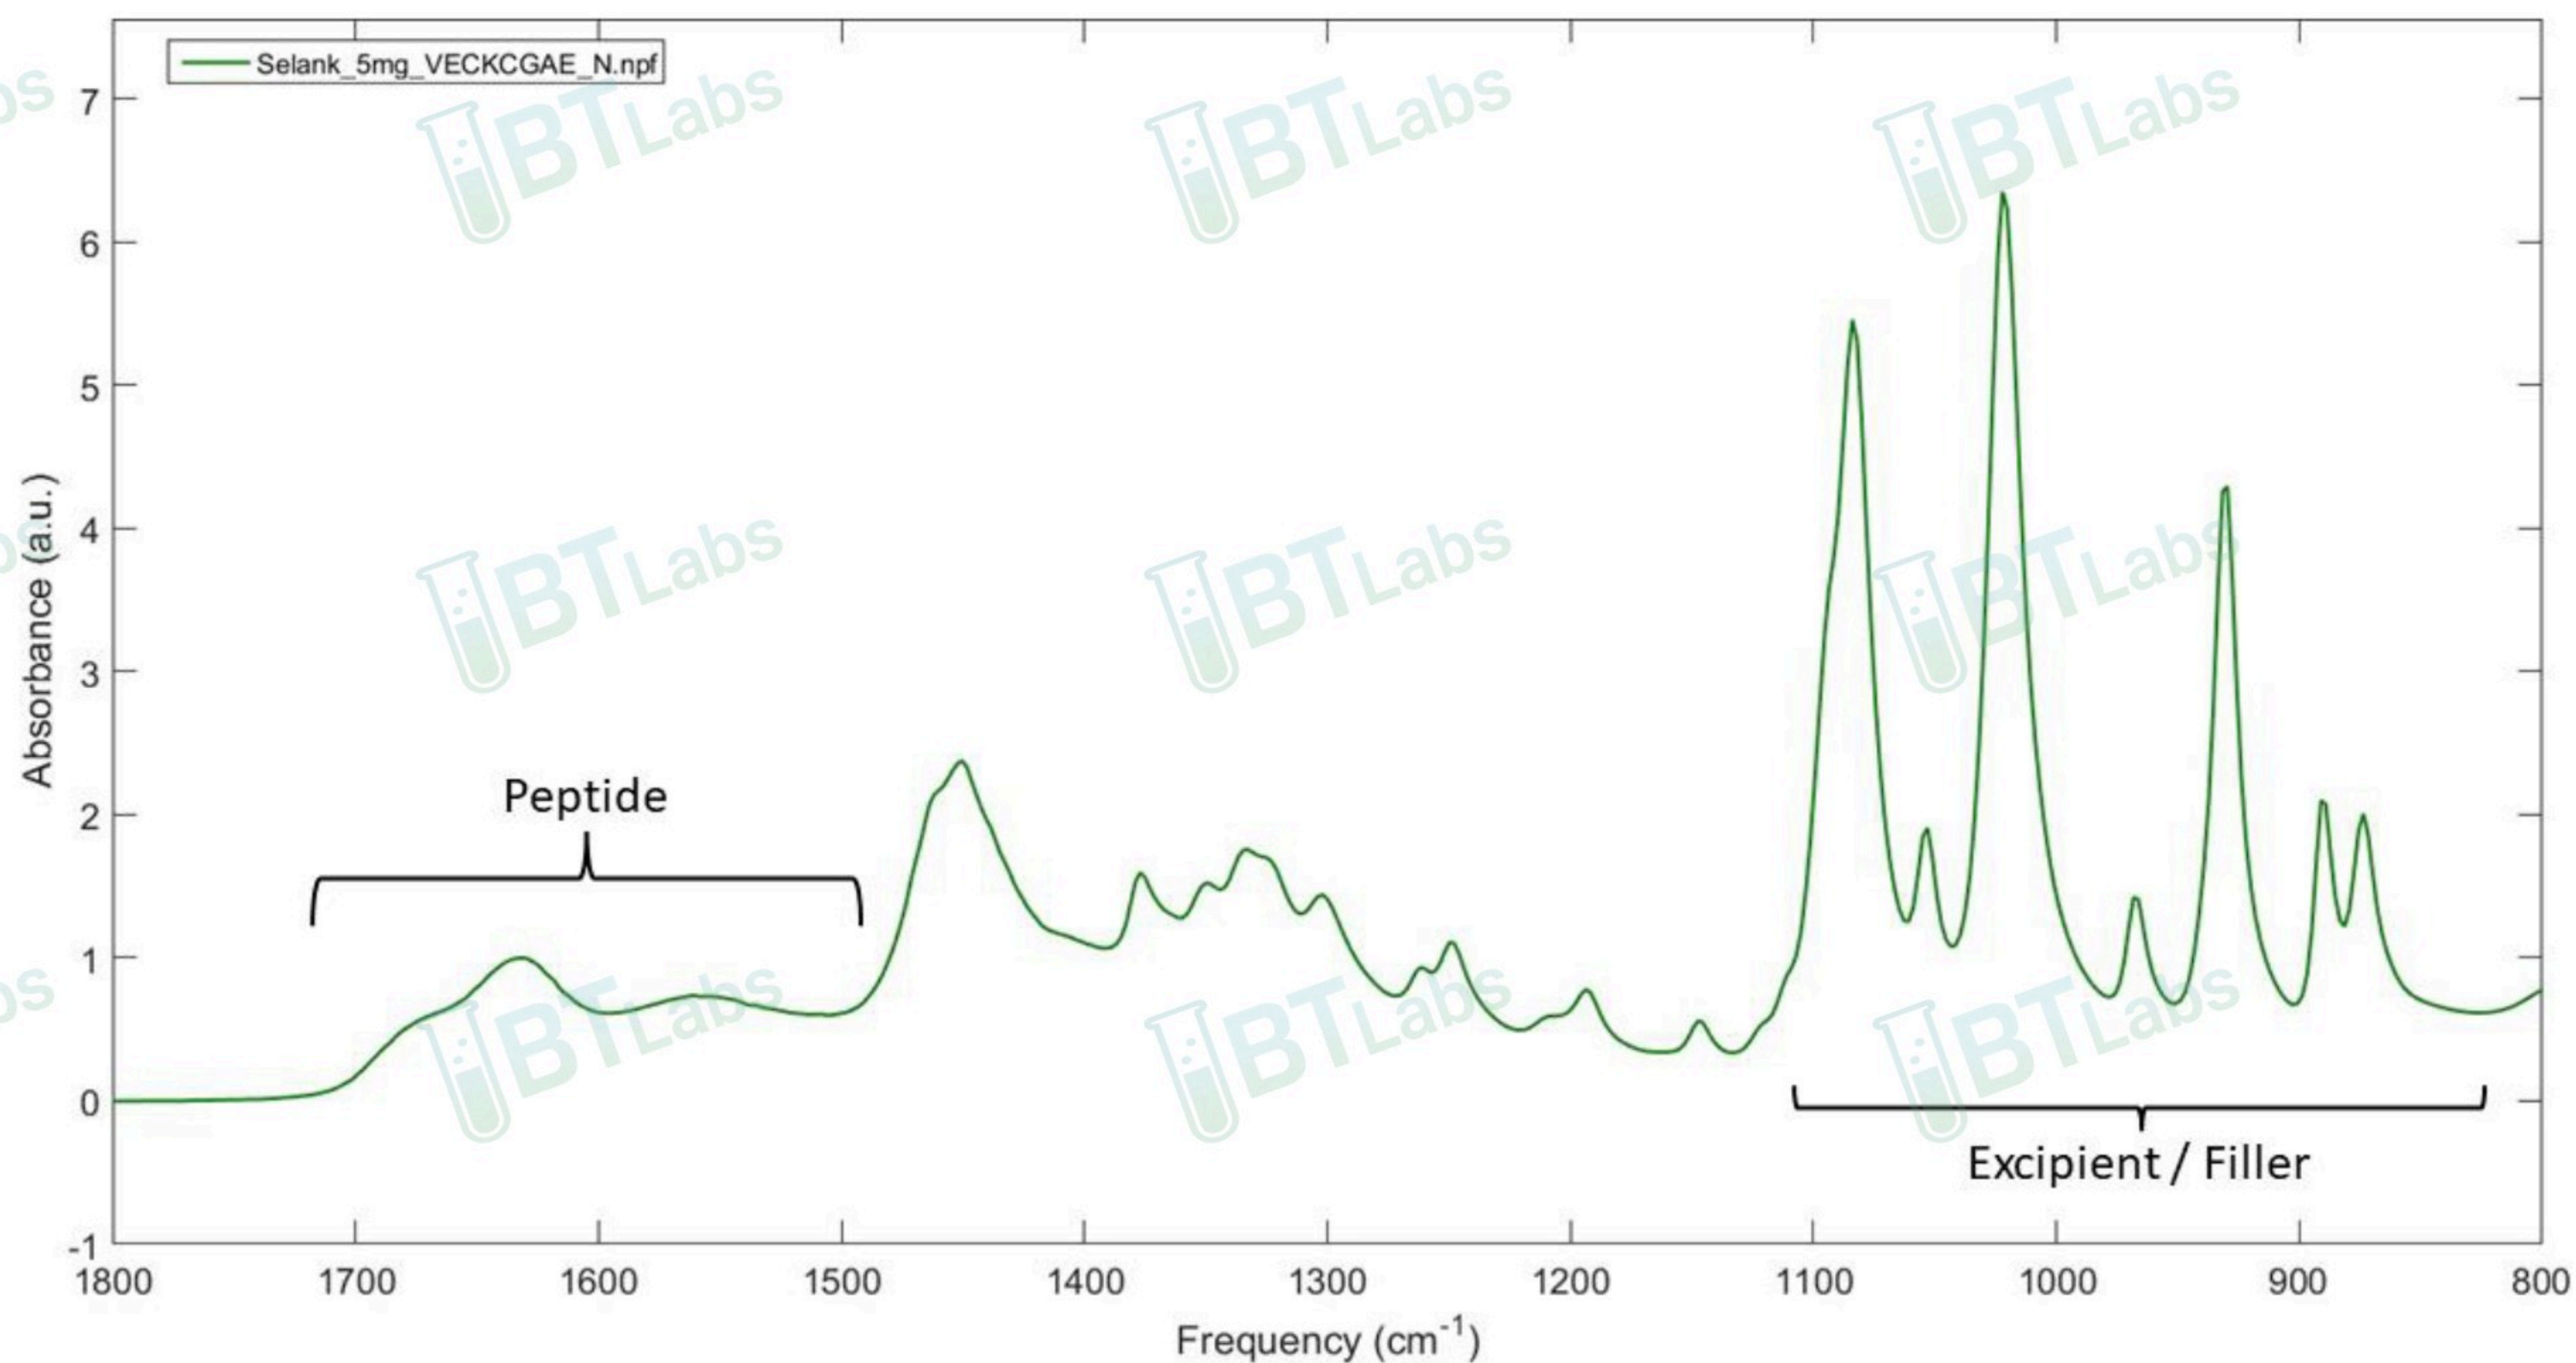

HPLC Purity and Potency Assay @ 220 nm: Selank Lot VECKCGAE

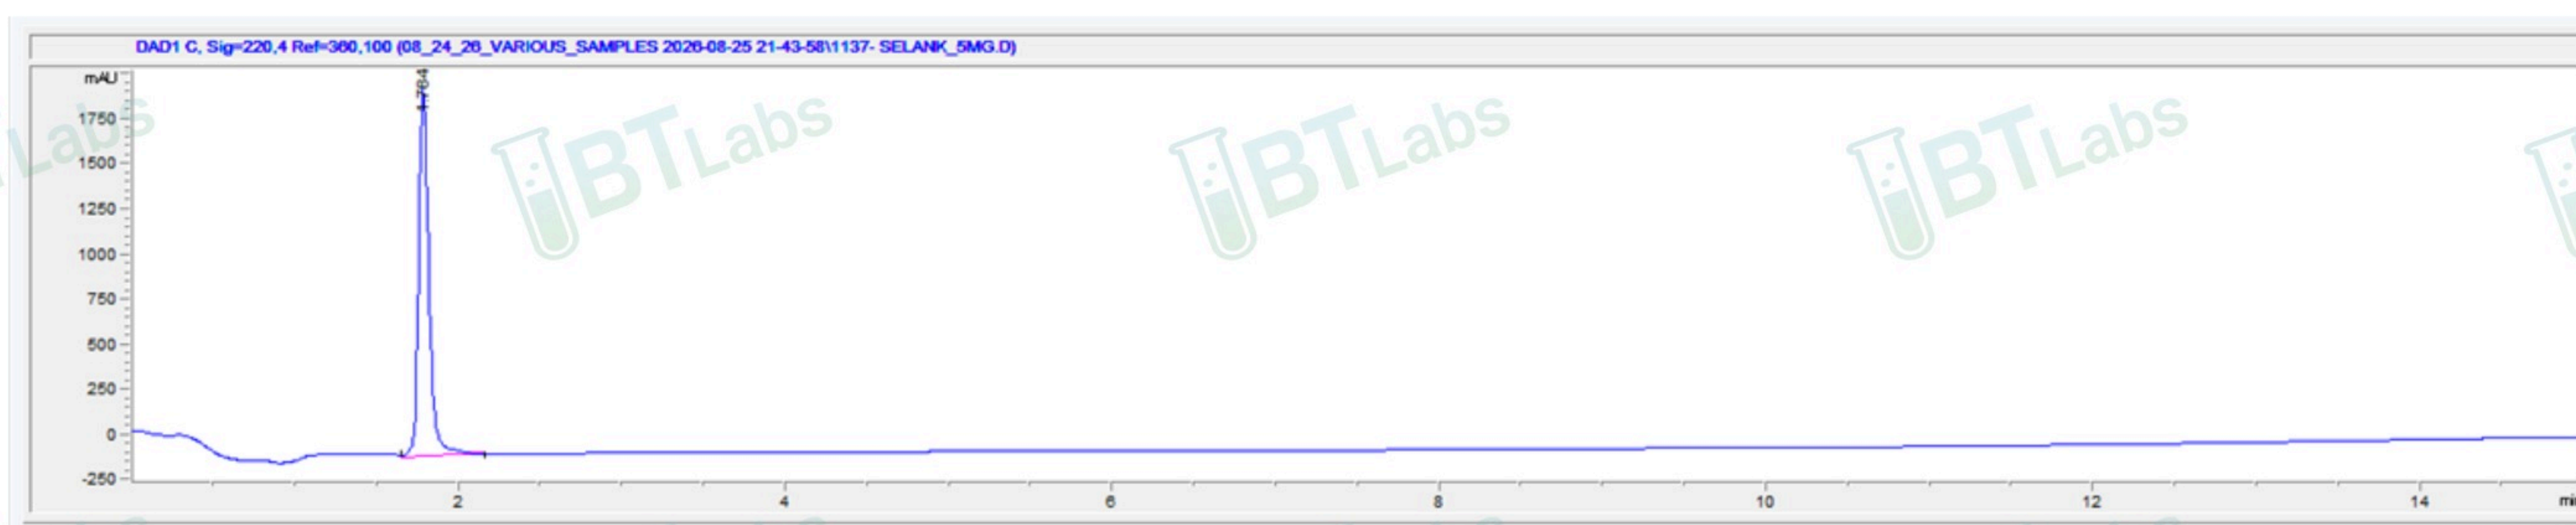

Selank Lot VECKCGAE @ 220 nm		
Peak #:	Retention Time (min)	Area (mAU*s)
1	1.784	9012.9